Instruction Manual

Manual Wheelchair

SectorCare®

WCP1H

Contents

Introduction

01 Safety Instructions 01

02 Installation Guide 02-04

03 Usage Operation 05-06

Safety Instructions

Please read this user manual carefully before using the manual wheelchair.
Keep this manual for future reference. If you do not fully understand the instructions, warnings, or precautions in this manual, consult your dealer or a qualified technician before using the product. Improper use or incorrect installation may result in injury.

When using the product, basic safety precautions should always be followed:

1. Press seat cushion to lock crossbar into frame slots.
2. Fasten seat belt if physical control is limited.
3. Slow down on turns and slopes to prevent tipping.
4. Ensure both feet rest on the footrests when moving the wheelchair.
5. Keep fingers away from the top and bottom of the support tube to avoid injury.
6. When ascending stairs, the assistant should press the lower rear tilt lever and lower the push handle to lift the front wheels onto the stairs.
7. Use the brake to lock the wheelchair when parked to prevent movement.
8. Apply both brake handles together to slow down and maintain control.
9. Do not slide downhill or brake suddenly during fast driving.
10. Avoid stepping on pedals when entering or exiting to prevent tipping.
11. Do not overinflate tires to avoid discomfort or blowouts on bumps.

Installation Guide

Major Parts

Congratulations on your purchase of our products. Our Manual Wheelchair are manufactured from the finest materials and components available, and to meet our own highly rigid specifications and will surpass your expectations.

01 Back Push Handle

02 Brake Handle

03 PU Armrest

04 Breathable Seat Cushion

05 Parking Brake

06 Footrest

07 12 Inch Solid Back Wheel

08 6 Inch Solid Front Wheel

09 Headrest

Installation Procedure

1. Remove the wheelchair and spare parts from the packaging. Wheelchair in folded position.





2. Pull the backrest backward and press down on the front of the seat until the wheelchair is fully opened.

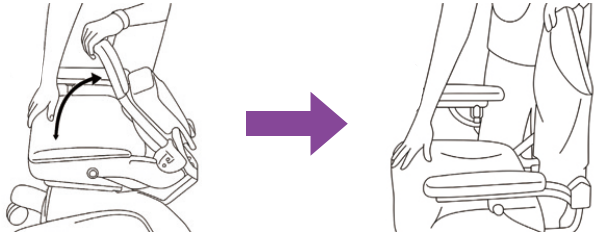

3. Place the lock ring into the slot, then press the switch lock plate firmly. (Note: The wheelchair cannot be used if the switch is not locked.)

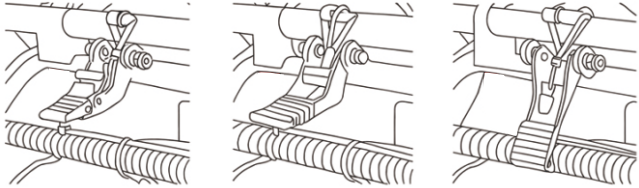

4. Wheelchair unfolding completed.

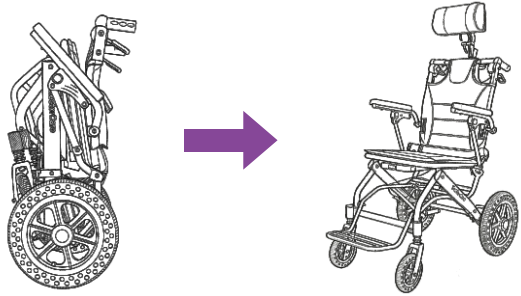

Usage Operation

Folding Procedure

1. Switch lock operation: First, lift the switch lock plate firmly, then remove the lock ring and place it below to fold the wheelchair.

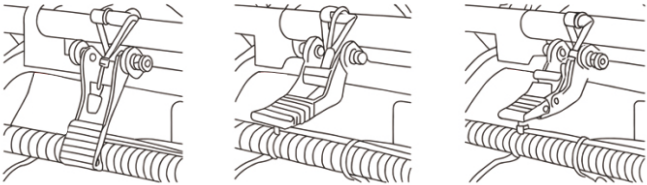

2. Hold the backrest tube and the front underside of the seat, lift both toward the center simultaneously, and fold the wheelchair.

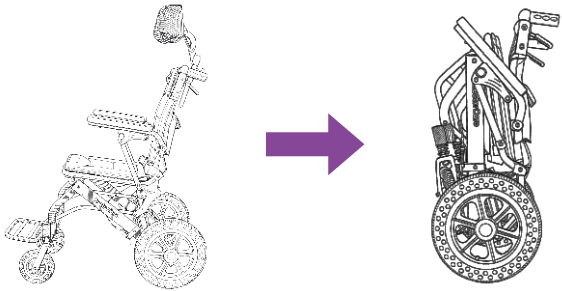

Method Of Getting On And Off

1. Lift the foot pedal, apply the brake, hold the armrest, and enter slowly. Set the pedal flat after sitting.
2. Park, apply brake, lift the pedal, hold the armrest, and exit slowly. Do not step on the pedal.

Shock Absorption System

1. The front shock absorption system absorbs bumps and vibrations, ensuring a smoother ride. It improves traction and braking on uneven terrain.

2. The rear shock absorption system enhances stability, reduces jolting, and lessens impact on the spine and back for greater comfort. It also improves performance on rough or uneven surfaces.

LEGAL STATEMENT

This manual and its contents are protected under the Copyright Act 1968 (Cth). No part of this publication may be reproduced, distributed, modified, stored in a retrieval system, or transmitted in any form or by any means without the prior written permission of FRG Pty Ltd. Unauthorized use is strictly prohibited.

© 2026 FRG Pty Ltd. All rights reserved.

SectorCare®

https://sectorcare.com.au